


From chair to chair

1




Place sling around patient.
Place leg straps on the inside of thighs.
Make sure sling is not folded or twisted.

2

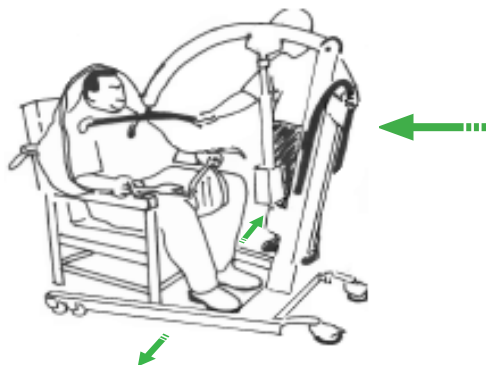


Position lift in front of patient. If needed, place patient's legs on or over the chassis.
Adjust spreader bar to shoulder height.

3

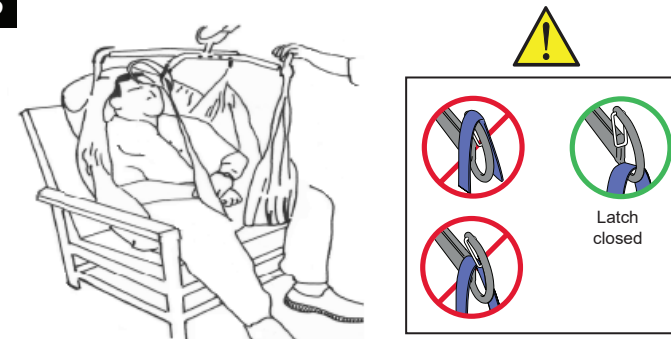


Attach sling loops to spreader bar correctly.
Make sure sling is secured in the hooks before lifting patient.

4

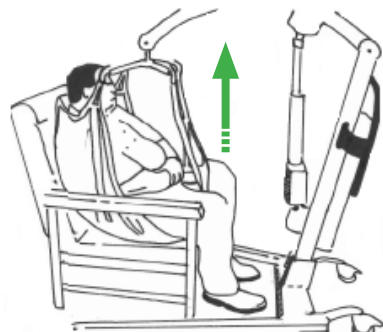


Lift patient.

5

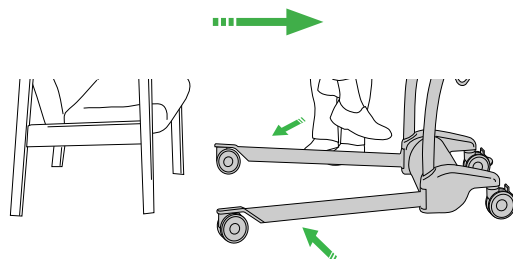

Move lift away from chair.
If applicable, close chassis legs.
Transfer patient.

6

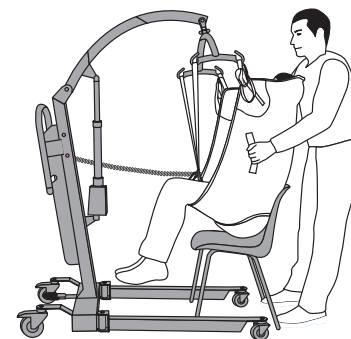

Position patient over chair. Carefully lower to sitting position.
Detach sling from lift. Move lift away from patient.
Remove sling from patient.